

Triton[®] DO80

Dissolved Oxygen Analyzer




ELECTRO-CHEMICAL DEVICES



Why choose a Triton® DO80?

- ❖ Easy to Use
 - Pre- Calibrated
 - No initial Burn In Required
 - No Liquids or Membranes to handle
- ❖ Easy to Calibrate
 - Zero,
 - Slope,
 - or Standardize
- ❖ Rugged design
- ❖ Fast Response
- ❖ Not flow sensitive





What is the Triton® DO80?

- ❖ The Triton® DO80 is an Optical Dissolved Oxygen Analyzer
 - Measures the Partial Pressure of oxygen in the water or air
 - The same O₂ measurement that is performed with galvanic or polarographic sensors.
 - With an improved technology
- ❖ Uses the Optical Property “**Fluorescence**” to determine the amount of oxygen dissolved in the water or present in the gas.





What is the Triton® DO80?

❖ The Triton® DO80 Sensor is a Smart Sensor.

- Digital Communication
- All data processing is internal to the sensor
- Calibration is stored in the sensor's memory
- Integral Temperature measurement
- Self diagnostics
- Easily replaceable sensor cap, greater than two year life is typical





What is the Triton® DO80?

- ❖ The Triton DO80® Analyzer has all the features of the T80 and can be ordered as a Single or Dual channel instrument.
- ❖ The standard model has
 - (1) 4-20 mA output per Channel
 - (3) relays
 - The digital communication of the Triton® DO80 limits the sensor choices to the DO80 sensors only.






Specifications


- ❖ Measuring Range
 - 0 - 20 mg/l (0 - 20 ppm)
 - 0 - 200 % Saturation
 - 0 - 400 hPa (0 – 400 mbar)
- ❖ Maximum Pressure
 - 10 bar (145 psi)
- ❖ Temperature Range
 - -5° - 50 ° C (20 ° - 120 ° F)
- ❖ Response Time
 - T90 < 60 seconds
- ❖ Accuracy
 - Max. error < 2% of measurement range
- ❖ Resolution
 - 0.01 mg/l or 0.01% SAT






How does it Work?

- ❖ Inside the sensor there is a **Green LED** light source that flashes rapidly.
- ❖ It Shines through a window on the inside of the membrane cap to the optically active layer.
- ❖ The layer contains organo-metallic (OM) molecules that **Fluoresce** red light when excited by the green light.
- ❖ A detector measures the intensity and response time (decay) of the **Fluorescence**.

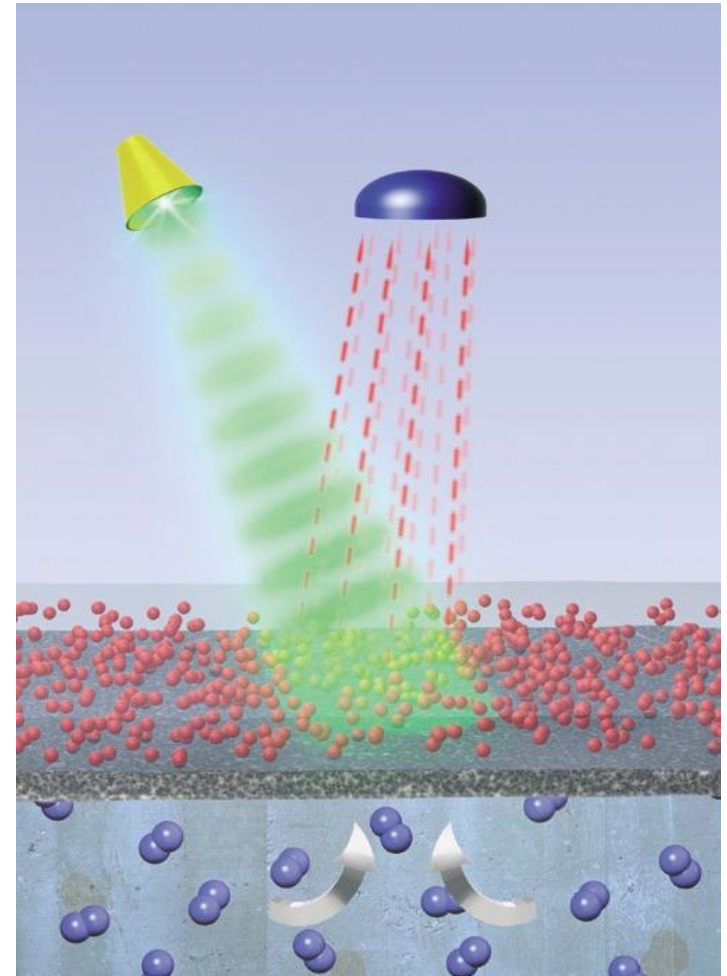





How does it Work?

- ❖ Oxygen exchanges freely between the media and the OM molecules in the cap.
 - A thin silicone coating protects the OM molecules from the environment.
- ❖ The OM Molecules catch and release the O_2 depending on the concentration present.
- ❖ When oxygen binds to the molecule, it fluoresces less.
- ❖ Hence the name of the technology **Fluorescence Quenching**.
- ❖ **No O_2 = High Fluorescence**
- ❖ **High O_2 = Low Fluorescence**

No O_2 , High Fluorescence

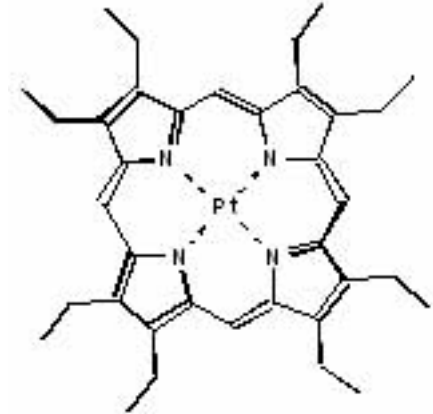


High O_2 , Low Fluorescence

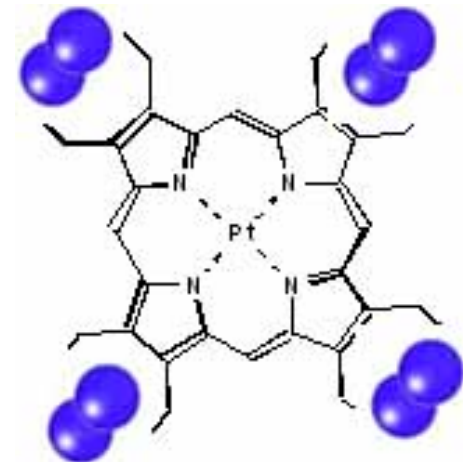



How does it Work?


- ❖ The amplitude of the signal, its intensity, is large and the response time of the decaying signal is long in low oxygen environments.
- ❖ The amplitude is lower and the response time is shorter for higher oxygen environments.
- ❖ The **Amplitude and Response time are independent of each other.**
 - Response time is used to calculate the Oxygen concentration
 - Amplitude infers lifetime of the cap and the sensors dynamic range

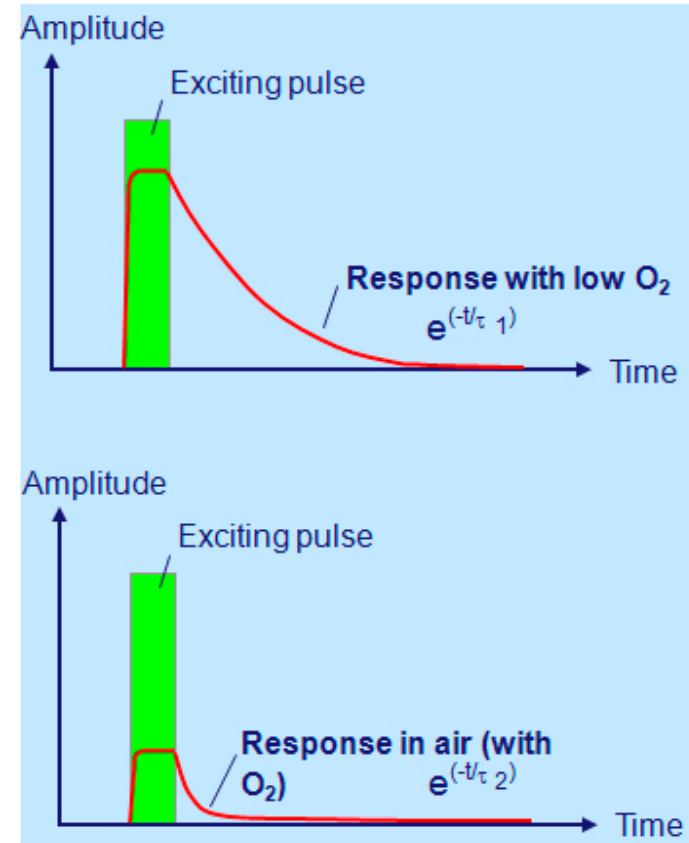



How does it Work?

- ❖ In Low Oxygen environments
 - Small changes in the oxygen cause large changes in the signal.
 - This leads to high noise and signal instability.
- ❖ In High Oxygen environments
 - Large changes in oxygen cause only small changes in signal.
 - The Changes become undetectable
- ❖ Optimal Measuring Range
 - 0.5 ppm low end
 - 15 ppm high end

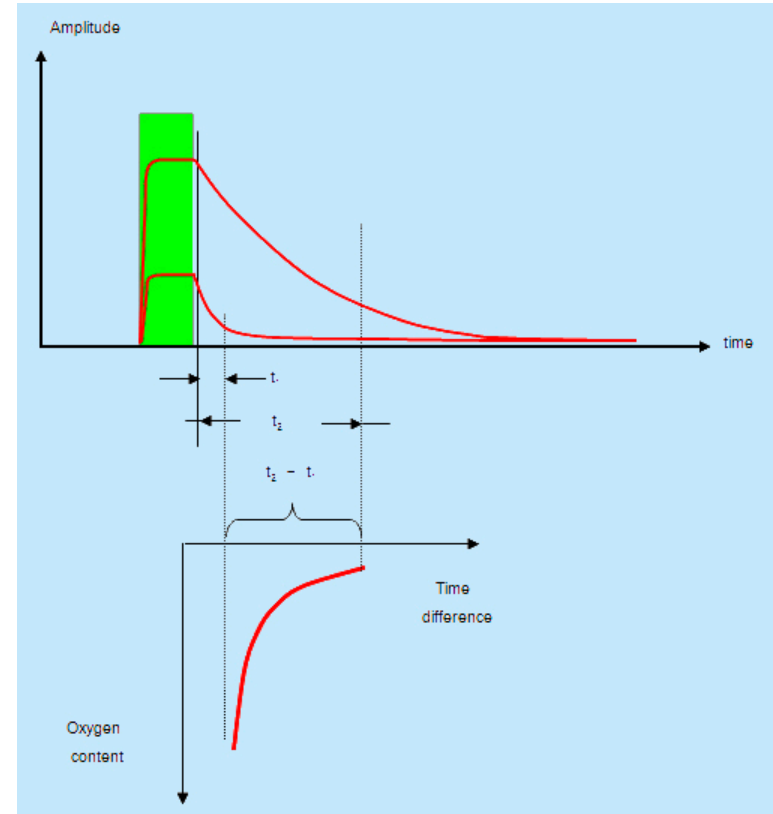



Where are they used?

- ❖ Municipal WWTP
 - Aerobic/Anoxic
 - Nitrification/Denitrification
- ❖ Municipal Potable Water
- ❖ Fish Farming
 - High density requires aeration
- ❖ Monitoring of Aerobic or Anaerobic Chemical Processes
 - Food processing WWT
 - Chemical/Petro WWT





ECD Triton® DO8

❖ What's Needed (one from each group)

- Single/Dual Channel Analyzer,
 - T80
- Single/Dual Channel Analyzer,
 - C22
- Triton® DO80 Sensor, 7 m cable
- Triton® DO80 Sensor, 15 m cable
- Flow Through Cell
 - (PN 1000219)
- Immersion Pipe Assembly
 - (PN 1000223)

❖ Spare Parts (recommended)

- Replacement Cap
 - (PN 2500207)
- O-ring set for Cap
 - (PN 1000225)
- Air Blast Spray Cleaner
 - (PN 1000226)






Installation Assemblies

- ❖ Air Blast Cleaner
 - PN 1000226
- ❖ Immersion Assembly
 - PN 1000234-xx(3-10 ft)
 - PN 1000234-99 (user supplied 1" pipe)
 - Does not include Mounting Brackets
- ❖ 3/4" NPT Flow Through Cell
 - PN 1000219-1
- ❖ 2" NPT Ball Valve Insertion Assembly
 - PN 1000251-2





Electro-Chemical Devices

Thank You,

Go to www.ecdi.com for Data Sheets/ Instruction Manuals/ Presentations/ Press Release Packages

For over 30 years Electro-Chemical Devices (ECD) has been a recognized leader in industrial process instrumentation:

Liquid analytical sensors, controllers, transmitters, analyzers and electrodes.

Electro-Chemical Devices
1681 Kettering
Irvine, CA 92614

Phone: +1-949-336-6060
+1-800-729-1333
Fax: +1-949-336-6064
email: sales@ecdi.com
web: www.ecdi.com

